
# Turner PRO

## @etac\*

EN - User manual IT - Manual utente
DE - Gebrauchsanweisung FR - Manual d`utilisation
NO - Brukermanual ES - Manual de usuarioo
SV - Bruksanvisning NL - Handleiding

FI - Käyttöohje DK - Brugsvejledning

BM61099 RevG 2021-12-29

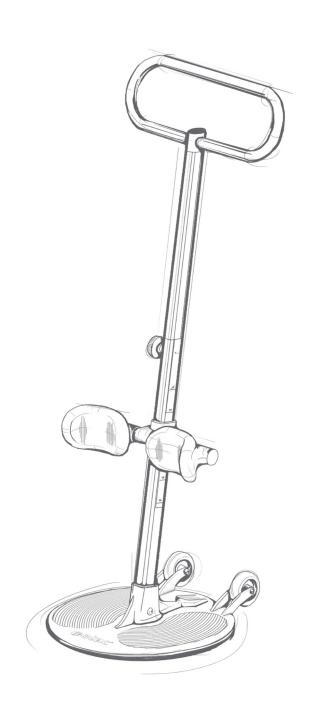







## Contents

l	lser	manua	l -	Ena	lis	h -	4

Bruksanvisning - Svenska - 8

Brukermanual - Norsk - 12

Brugsvejledning - Dansk - 16

Käyttöohje - Suomi - 20

Gebrauchsanweisung - Deutsch - 24

Handleiding - Nederlands - 28

Manual d'utilisation - Français - 32

Manual utente - Italiano - 36

Manual de usuarioo - Español - 40

#### General

#### CEdeclaration



The product, and its related accessories, described in this instruction for use (IFU), is in compliance with the regulation (EU)2017/745 of 5. April 2017 – as a medical device, risk class I. The product is manufactured and tested according to EN12182:2012 and selected parts of EN/ISO10535:2006.

Any serious incident that occurs in relation to the device should be reported to the manufacturer and the competent authority of the Member State in which the user and/or patient is established.

#### Conditions for Use:

Transferring a person may pose an element of risk. Only trained personnel should use the equipment covered by this user manual. Warranty notice

Two-year warranty against defects in workmanship and materials of our products.

Pleaserefer to www.etac.com for terms and conditions.

Visit www.etac.com to download the latest version of our doccumentation.

#### **Important**

This User Manual contains important safety instructions and information regarding the use of the Turner PROand accessories. In this manual the user is the person being transferred. The assistant is the person operating the Turner PRO.



This symbol indicates important information related to safety. Follow these instructions carefully.



Read User Manual before use!

It is important to fully understand the content of the user manual before attempting to use the equipment.

Modifications and use of components made by other manufacturers:

We recommend only using Etac components and spare parts. Declaration of conformity is not valid and Etacis not responsible for warranty if any modifications are made to the product. Etac shall not be liable for faults or accidents that can occur when using components made by other manufacturers.

#### Risk assessment

Assessthe risk and take notes.

You as the assistant are responsible for the safety of the user!



Only technical personnel are allowed to perform repairs.

#### Labels and symbols

#### Product label:

The label contains art. number and serial number (bar codes). The EAN code contains;

- (01) (EAN no.): xxxxxxxxxxxxxx
- (11) (Batch): YYMMDD

Short user quide:

li

(21) (Serial number): xxxxx



#### Symbols:

Symbols used on the product, explained in more detail:



Manufacturer



Date of manufacture



Catalogue number





Serial number



Medical Device



CE marked



Refer to user manual



Max temperature when washing



lax userweight (SWL)



pH when washing




QR code

#### Turner PRO- intended use

Turner Prois a sit-to-stand transfer aid that makes it easier for a carer to help a user to stand and transfer him/her to another sitting position. Usersmust be able to grip and pull up their own body weight, but still require support/help to stand up and be turned. The purpose is to transfer a person from/to bed, chair, wheelchair or toilet. The Turner PROislightweight and easy to move around. The Turner PROshould only be used indoor on flat surfaces.

## Turner PRO

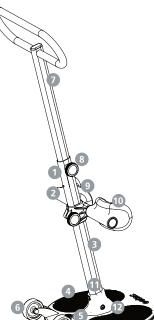

- 1. Outer pole
- 2. Lock pin
- 3. Height label
- 4. Main plate
- 5. Assistant footrest
- 6. Transport wheels
- 7. Inner pole with handle
- 8. Turning knob
- Short user guide
- 10. Leg support
- 11. Product label
- 12. Bolts

## Technical data

Safe Working Load (SWL): 200 kg (441 lbs) Weight of unit:

8kg

Dimensions:

Height(A): 0,8-1,2 m 0,3-0,55 m Height (B):


Depht (C): 0,46 m With (D): 0,45 m Footplate (Ø): 0,40 m


#### Material:


Powder coated aluminum, Plastic, Steel.


#### Expected Lifetime:

The Turner PROhas an expected lifetime of 5 years or 15000 turning cycles

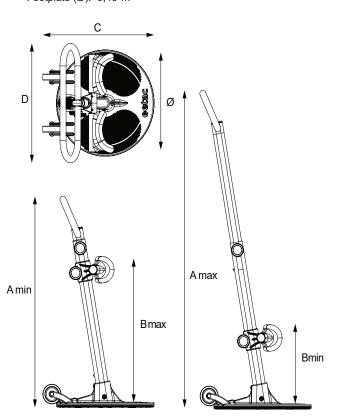

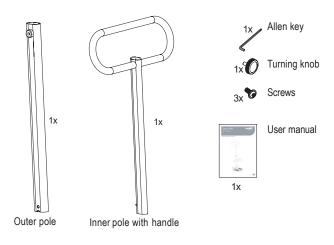







## Mounting leg support

The knee cushions are adjusted individually. The leg support has step-less adjustment from 0,3 to 0,55 meters. Follow these two steps when mounting the leg support:




Lay the pole down on an even surface. Insert leg support with kneepads pointing upwards. Make sure both knobs are on the same side.




Tighten knob by turning knob clockwise.

#### Mounting pole to main plate








Place the base plate on an Insert all three screws into holes in the base plate. Use allen key to screw in bolts. Tighten bolts firmly.




Make sure that all three bolts are properly fastened. Loosebolts can make the pole wobbly and the Turner PROunsafe to use.

## Mounting handle


The handle has step-less adjustment from 0,8 to 1,2 meters. Follow these three steps when mounting the handle:



Placethe handle with the lock-pin pointing towards the wheels.



Pressin the lock pin and slide the pole into the mounted pole.



There will be a clicking sound when it is correctly mounted. Turn and tighten the knob.

#### Checklist after assembly




Don't start using Turner PRObefore completing the checklist after assembly.


Use this checklist to verify that the Turner PROis properly installed and can operate correctly and safely before use. Seeassembly information on the previous page for details.

- † Make sure that the leg support is mounted correctly.
- † Make sure that all three bolts between outer pole and main plate are mounted correctly and properly tightened.
- † Make sure that the handle (inner pole) is mounted correctly.
- † Make sure Turner rotates freely.


## Adjusting handle height



Turn knob counter clockwise and adjust handle height.



Pushthe lock pin in if the handle is in upper position.



When correct handle height is obtained, turn knob clockwise to lock the position.




Be aware of handle when adjusting height. Handle can slide down and hit operators head or upper body.




Don't use handle in a position above the lock pin position. This makes the pole wobbly and the Turner unsafe to use.


## Adjusting leg support height



Turn knob anti clockwise and adjust knee support height.



When correct knee support height is obtained, turn knob clockwise to lock the position.



The knee support height can be read from the scale on the pole. The number above the leg support bracket referes to the correct height.




Make sure knobs are securely tightened. Lose knobs can cause handle or knee support to slide down and make the Turner unsafe to use.


#### Positioning Turner PRO




Position the new seat (chair, wheelchair, toilet or bed) in an 90 degree angle with the existing seat.



Slide the Turner PROin under the users feet.



Adjust the height of the leg support so it is positioned two fingers beneth the users knee cap.



Adjust the height of the handle to a position that is comfortable for both user and assistant.

## Transport and storage

Turner PROcan be stored and transported under temperatures between -25 - 70  $^{\circ}\text{C}$  and relative humidity between 15 - 93 %









Don't use the Turner Pro for transportation of people or goods.

## Transfering user







Encourage the user to stand up, at the same time, counter-balancing the users weight using a foot and hands (use your bodyweight by leaning backwards).





Twist the Turner PROso that the user is transferred to the front of the new seat.



Step on footrest, brace your weight and ask the user to sit down. Maintain eye contact with the user during the entire transfer prococess.


#### User / Assistant








The assistanthas to be able to handle the weight of the user.







Make sure the users weight is within the baseplate.

## Cleaning and disinfection

Clean on a regular basis. Clean surfaces with a damp cloth using an appropriate pH-neutral detergent. Do not use solvents or strong liquids, this may damage surfaces on the Turner. For disinfection when needed; use isopropyl alcohol or similar. Avoid abrasive cleaning products. Remove hair and pile from the wheels and verify that the wheels rotates freely.



Make sure not to damage or remove labels when cleaning.

#### Reconditioning

Follow cleaning and assembly procedure. Separate reconditioning document is available at Etac.com.

## Recycling

Turner PROcan be disposed of as metal waste. Recycling instructions is available at Etac.com

## Spare parts

A list of spare parts is available at Etac.com.



Etac A/S Parallelvej 3 DK-8751 Gedved www.etac.com @etac\*